

User Manual

Gelida 47 | Version: v1



GENERAL INFORMATION

Copyright

This user manual and all contents contained herein are subject to copyright. All rights reserved. No part of this user manual may be reproduced, copied, translated or transmitted in any form or by any means without the prior written approval of Genea Biomedx.

Technical Support

Manufacturer

If any serious incident has occurred in relation to this device, it should be reported directly to the manufacturer and the competent authority of the Member State in which the user and/or patient is established.

**Genea Biomedx Pty Ltd**

Level 2, 321 Kent Street
Sydney, New South Wales, 2000, Australia

Country of origin: China

Email: info@geneabiomedx.com

Web: www.geneabiomedx.com

Authorized European Representative

**DONAWA LIFESCIENCE CONSULTING SRL**

Piazza Albania, 10
00153 Rome
Italy



Introduction

We appreciate your selection of Gelida 47 provided by Genea Biomedx Pty Ltd.

The User Manual provides handy, easily understandable guidance regarding the operation and maintenance of the product, including but not limited to, vital safety instructions, installation procedures, usage protocols, and maintenance information.

It is the owner's responsibility to ensure that all users of the Gelida 47 have read and understood this user manual before operating the instrument. Please carefully read the User Manual before operation to ensure the proper use of this product.

Keep the User Manual for quick reference in case of any issues. Any further updates or changes to the User Manual shall be incorporated into supplemental or specialized training.

Notice: reading the manual does not automatically confer the authority or demonstrate the competence to use this product.

Product configuration:

Gelida 47 is offered in two configurations with 4 product codes, as shown below:

Code	Description
GELI-01-US	Gelida 47L - Canister Variant (US only)
GELI-02-US	Gelida 47L - Rack Variant (US only)
GELI-01-CE	Gelida 47L - Canister Variant (CE only)
GELI-02-CE	Gelida 47L - Rack Variant (CE only)

List of accessories

No.	Content	GELI-01-CE/GELI-01-US	GELI-02-CE/GELI-02-US
1	Liquid nitrogen storage tank	1	1
2	Canister	10	/
3	Rack	/	6
4	Insulation cap /plug	1	1
5	User Manual / IFU	1	1
6	Power adapter	1	1

No.	Content	GELI-01-CE/GELI-01-US	GELI-02-CE/GELI-02-US
7	Charging cable	1	1
8	Battery	1	1
9	Emergency Key	1	1
10	Tag	1	1
11	Roller Base	1	1
12	Supporting Documents	1	1

In case of any missing accessories, please promptly contact your local Genea Biomedx representative. This product does not contain any parts that are prone to wear and tear or loss. The accessories require replacement only in the event of damage.

***Note:** In some cases, the “User Manual” can be obtained digitally as an eIFU; please contact your local Genea Biomedx representative to get the latest version of the User Manual.

Copyright description

This manual contains proprietary information protected by copyright law. All rights reserved.

Reproduction, photography, or translation of any part of the Manual into other languages is prohibited without the express written consent of the manufacturer.

See the nameplate for the date of manufacture for the device.

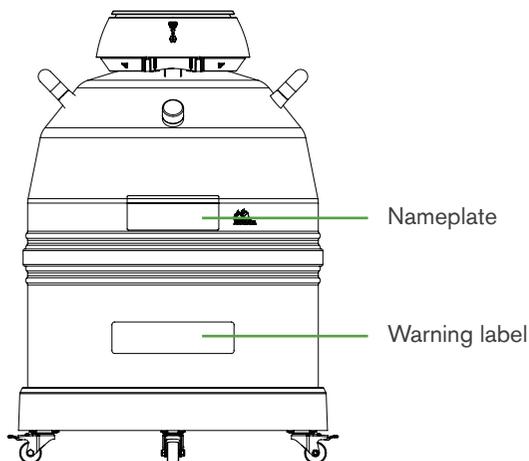


Table of contents

1. Introduction	1
1.1 Product Overview	1
1.2 Intended Use	1
1.2.1 Indications for Use	1
1.2.2 Patient target group	1
1.2.3 Intended users	1
1.3 Device Structure & Key Features	2
1.4 Contraindications	2
1.5 Technical Data and Performance Characteristics	2
1.6 Shipping, Unpacking & Inspection	3
1.7 Conditions for Operation & Storage	3
1.8 Safety & Precautions	4
1.9 Definition of icons, symbols and abbreviations	7
2. Use of Gelida 47	9
2.1 Product structure	9
2.1.1 Layout & Configurations	9
2.2 Included accessories	12
2.2.1 Emergency Key	12
2.2.2 Battery	13
2.2.3 Power supply	14
2.2.4 Power adapter and charging cable	14
2.2.4.1 Charging	14
2.2.4.2 Replacing the battery	15
2.2.5 Insulation plug	17
2.3 Product setup & installation	18
2.3.1 Installation space	18
2.3.2 Installation method	19
2.3.3 Opening the Tank Lid	20

2.3.4 Filling Liquid Nitrogen	20
2.4 User operation	22
2.4.1 Turning on and using the Display	23
2.4.2 Warning & Faults Management	23
2.4.3 User Password Modification	24
2.4.4 System Access Logs	25
2.4.5 Alarms & Muting Alarms	26
2.4.6 Lid operation	26
2.4.6.1 Unlocking lid	27
2.4.6.2 Locking lid	27
2.4.7 Sample access	28
2.4.7.1 Accessing a Canister/Rack & Sample	28
2.4.7.2 Replacing a Canister/Rack & Sample	29
2.4.8 LN2 Liquid Level Estimate	30
2.4.9 Temperature Display	31
2.4.10 Battery Level Display	32
2.4.11 Settings	32
2.4.11.1 Wi-Fi & IP settings	33
2.4.11.2 Date & Time Setup	34
2.4.11.3 User management	34
2.4.11.4 Administrator password modification	36
2.4.11.5 Language	37
2.4.11.6 Alarm Temp of the Upper Probe (°C)	38
2.4.11.7 Alarm Temp of the Lower Probe (°C)	38
2.4.11.8 Lid Open Time (Min) Before Alarm	38
2.4.11.9 Screen brightness (%)	38
2.4.11.10 Volume Adjustment (%)	38
2.4.11.11 GPS Location	38
2.4.11.12 Wi-Fi toggle	39
2.4.11.13 Single/dual password verification	40

2.4.12 "Find My Tank" Function	41
3. Technical Specifications	42
4. Product Maintenance & Support	45
4.1 Product Service Life	45
4.2 Routine maintenance & calibration	45
4.2.1 Temperature Calibration	45
4.2.2 Defrosting the Tank	45
4.2.3 Tank Inspection & Monitoring	45
4.2.4 Decontamination	46
4.3 Device Disposal	46
4.4 Warnings & Faults: Troubleshooting	47

1. Introduction

1.1 Product Overview

The Gelida 47 is a state-of-the-art liquid nitrogen storage system provided by Genea Biomedx Pty Ltd. It is specifically designed for use in hospitals, clinics, laboratories, or research units.

Gelida 47 addresses the critical need for long-term, static sample storage with a focus on providing robust, efficient, and intelligent monitoring capabilities, thereby mitigating the risk of biological sample degradation. For sample preservation, the protocol involves placing the samples in designated storage containers, which are then securely placed within liquid phase LN2 within the Gelida 47 tank for effective cryogenic preservation

It offers real-time monitoring of internal temperature conditions. In instances of temperature deviations beyond user set thresholds, the system promptly initiates alert and user notification mechanisms. Two temperature sensors, placed in the upper and lower portion of the tank, allow for the platform to infer liquid nitrogen levels within the Gelida 47 system. Audio and visual alarms are emitted from the tank lid. Additional remote alarms & notifications are provided via Wi-Fi connection to external monitoring software sold separately.

Access to samples within the tank are protected by a user associated password, which connects to an electromechanical lock; it safeguards against unauthorized manipulation of the stored samples, and provides traceability of tank access, thus ensuring their integrity and safety.

1.2 Intended Use

This product is designed for prolonged cryogenic preservation & storage of laboratory samples like cells, tissues, and other biological samples. Storage is at extremely low cryogenic temperatures using liquid nitrogen.

1.2.1 Indications for Use

No condition treated. Device is intended to facilitate low temperature storage of biological samples in a laboratory or clinic environment.

1.2.2 Patient target group

No therapy is applied to any patients. The tank is used to store biological samples in liquid nitrogen. Gelida 47 parts or accessories do not interact directly with any patients for their function.

1.2.3 Intended users

Laboratory Professionals in hospitals, clinics, laboratories, or research institutions environment.

1.3 Device Structure & Key Features

The Gelida 47 consists of a vacuum insulated liquid nitrogen storage tank, with a smart lid. The smart lid incorporates connected temperature sensors, a control/monitoring system, Wi-Fi connectivity, a display screen, a digital electromechanical lock, and an audible alarm system.

1.4 Contraindications

There are no known contraindications.

1.5 Technical Data and Performance Characteristics

Refer to specific product specification sheet in Section 3 or contact Genea Biomedx for further information.

Standards Compliance:

Electrical safety:

The system is designed, inspected, and tested in accordance with EN 61010-1:2010+A1:2019 Safety requirements for electrical equipment for measurement, control, and laboratory use -- Part 1: General requirements, as well as IEC 61010-1:2010+AMD1:2016 Safety requirements for electrical equipment for measurement, control, and laboratory use -- Part 1: General requirements.

Electromagnetic Compatibility:

EN IEC 61326-1:2021 Electrical equipment for measurement, control and laboratory use - EMC requirements -- Part 1: General requirements

Radio Frequency:

Changes or modifications not expressly approved by the party responsible for compliance could void the user's authority to operate the equipment.

NOTE: This equipment has been tested and found to comply with the limits for a Class A digital device, pursuant to part 15 of the FCC Rules. These limits are designed to provide reasonable protection against harmful interference when the equipment is operated in a commercial environment. This equipment generates, uses, and can radiate radio frequency energy and, if not installed and used in accordance with the instruction manual, may cause harmful interference to radio communications. Operation of this equipment in a residential area is likely to cause harmful interference in which case the user will be required to correct the interference at his own expense.

1.6 Shipping, Unpacking & Inspection

The Gelida 47 from Genea Biomedx are supplied in new condition. For your own protection, schedule enough time to check for any external damage on delivery. Mishandling of the device, including transport and shipping of units in non-approved orientations, may damage the product and contents. If the tank experiences a sufficiently severe drop or impact, it may result in tank failure.

Open the freight container and check that all items are present. Record all components on the packing list before disposing of any transport material. Contact the logistics carrier and your local Genea Biomedx Distributor/Representative if there are signs of shipping damage or any missing items.

1.7 Conditions for Operation & Storage

Usage environment

Usage site:	Well-ventilated indoor area.
Altitude:	Below 2,000 meters.
Environmental temperature:	+5°C to +40°C.
Environmental humidity:	20% RH to 80% RH, non-condensing.

Storage environment

Environmental temperature:	+5°C to +40°C.
Environmental humidity:	20% RH to 80% RH, non-condensing.

Transport Environment

Environmental temperature:	+5°C to +40°C.
Environmental humidity:	20%RH to 80%RH, non-condensing.



NOTE:

For safe transportation, always maintain the tank in an upright position. Securely fasten the system to prevent any movement or overturning. To absorb any impacts, place sponge or similar shock absorbing material at the base.

1.8 Safety & Precautions

This product is to be used only by personnel trained by the manufacturer. It is the owner's responsibility to ensure that all users of Gelida 47 have read and understood these warnings and cautions before operating the instrument. The protections and warranties provided with the product may be voided if the product is not used in accordance with the methods specified herewith in.

It is the owner responsibility to validate the device to ensure safety to items prior to use.

	<p>WARNING:</p> <p>It is the owner's responsibility to ensure that all users of Gelida 47:</p> <ul style="list-style-type: none"> • are trained in all laboratory safety procedures, including the handling of hazardous materials; • have read and understood the instructions and warnings contained in this user manual; • have received adequate training in the correct operation of instrument.
     	<p>WARNING:</p> <p>Liquid nitrogen is extremely cold. To avoid injury by frostbite, use extreme care whenever handling liquid nitrogen, liquid nitrogen storage or transfer vessels, or any objects which have come in contact with liquid nitrogen.</p> <ul style="list-style-type: none"> • Appropriate cryogenic protective gear must be worn to prevent cryogenic burns; leave no areas of skin exposed. <ul style="list-style-type: none"> ◦ Safety attire over clothing ◦ Face shield ◦ Cryogenic gloves ◦ Cryogenic apron • Use extreme care to prevent spilling and splashing liquid nitrogen during transfer. • Always keep vessel in upright position. Do not tilt or lay the vessel on side. • Get immediate medical attention for any frostbite injuries due to liquid nitrogen. • Immediately remove any clothing or safety attire on which liquid nitrogen has spilled. • When refilling with liquid nitrogen, pre-cool the system with a small amount of liquid nitrogen before refilling. The refilling process should be gradual to avoid splashing and potential cryogenic burn related injuries.
	<p>WARNING:</p> <p>Do not store or use container in areas that are small and enclosed or have poor ventilation. The venting of nitrogen gas may deplete oxygen in the air, possibly leading to asphyxiation or even death. It is recommended to add an oxygen concentration monitor and alarm in the tank room for additional user safety. It is recommended to add an oxygen concentration monitor for environmental monitoring.</p>
	<p>WARNING:</p> <p>Do not tightly seal liquid nitrogen container or prevent nitrogen gas from escaping. Avoid excessive humidity levels or exposure to liquid ingress that could result in freezing of the insulation plug, and possible explosion.</p>

	<p>CAUTION:</p> <p>Do not force the insulation plug into place.</p> <p>Do not modify the insulation plug in any way.</p> <p>The insulation plug should be carefully aligned with the markings and inserted without force. Damage or modification to the insulation plug may result in degraded product safety and performance.</p> <p>If the insulation plug is damaged, excessive LN2 usage may occur, or in severe cases, excessive pressure may build up which could result in explosion. Transfer samples to a backup cryostorage solution and contact your local Genea Biomedx representative for support.</p>
	<p>WARNING:</p> <p>Never use a hollow tube to measure liquid nitrogen level. This could lead to thermal injury.</p> <p>The device is equipped with 2 temperature sensors which are used to approximate the liquid level in the tank.</p> <p>Contact local your Genea Biomedx representative if you need alternative methods to measure liquid nitrogen level.</p>
  	<p>CAUTION:</p> <p>Handle the cryopreservation vessel with care during use, failure to handle with care may impact the product safety and performance and may void warranty.</p> <ul style="list-style-type: none"> • Never overfill vessels with liquid nitrogen. Liquid nitrogen should always be below the bottom of the neck tube. Overfilling the tank may cause immediate or premature vacuum failure to occur. • Never ship Gelida 47 on its side or upside down. • Remove and insert inventories carefully. Do not scratch neck tube area. Scratches can cause premature vacuum failure. • Never tamper with or removing the vacuum valve as this may result in vacuum failure. • Never drop or hit the unit. • Never spill liquid nitrogen on or near vacuum valve. • Never leave the vessel in outdoor conditions. • Never place the unit near a heat source. • Never have items stacked on top of the product. • Performance data available for the instrument is based on static conditions only. Actual performance will vary upon the nature of use. Addition or removal of samples, addition on non-validated accessories, along with vibration will decrease the working duration of these products.
	<p>CAUTION:</p> <p>The vacuum valve is designed with a structure that allows for repeated air extraction. Tank vacuum maintenance should be carried out by the manufacturer or trained Genea Biomedx service representative.</p> <p>Customers are prohibited from attempting these procedures themselves to avoid negative impacts to the product's performance and avoid voiding warranty.</p>

	<p>WARNING:</p> <p>The Gelida 47 is exclusively designed to be used with liquid nitrogen ONLY and should not be used to store any other cryogenic substances.</p>
	<p>WARNING:</p> <p>Use only the original Genea Biomedx Gelida 47 parts with the Gelida 47. Substitutes from other products (e.g. insulation plug, canisters and rack holders) are not allowed.</p>
	<p>WARNING:</p> <p>To reduce the risk of electric shock:</p> <ul style="list-style-type: none"> • Liquids, including liquid nitrogen, must not make contact with the tank lid or electronics; doing so may result in electrical short circuits. • Do not attempt to repair or modify any part of the instrument; • Do not remove any of the instrument panels or covers; • Do not place the instrument where it will be exposed to excessive moisture; • Do not replace the supplied charging power cord and/or power adapter with an incorrect rated cord or adapter; • Connect the charging power adapter only to an electrical power source with the proper voltage and frequency; • Immediately replace the power cord if it becomes damaged, frayed, cracked or broken.
	<p>CAUTION:</p> <p>If a sudden increase in evaporation loss is found, or if excessive frost & condensation appears on the exterior surface of the product, this may indicate tank damage or loss of tank vacuum. Ensure that tanks are inspected on a regular schedule according to your lab protocol.</p> <p>In such cases:</p> <ul style="list-style-type: none"> • Stop using the product immediately and contact local service representative. • Do not remove frost with hard objects to prevent further damage to the tank. • If samples are stored, carefully and quickly move them to alternative cryogenic storage.
	<p>WARNING:</p> <p>Only authorised service personal should calibrate, repair or replace parts within the Gelida 47 or perform other service and repair activities.</p> <p>Attempting untrained repair may result personal injury, loss of product features and performance, or voiding of product warranty.</p>
	<p>CAUTION:</p> <p>When accessing frozen samples work quickly and carefully to avoid premature thawing and unnecessary sample loss.</p>
	<p>WARNING:</p> <p>Do not place or use instrument near a strong source of RF radiation (e.g., an unshielded radio frequency (RF) source). Doing so may interfere with the electronics and communication functionality of the instrument.</p>

1.9 Definition of icons, symbols and abbreviations

Definition of icons, symbols and abbreviations used on the labels of the product is as follows:

Sign	Description
	Indicates that caution is necessary when: <ul style="list-style-type: none"> • Operating the device or control close to where the symbol is placed. • The current situation needs operator awareness or operator action to avoid undesirable consequences.
	Indicates additional information which may assist in product use
	Unlock direction
	Charging port voltage
	Power button
	Indicates the device manufacturer
	Indicates the date when the device was manufactured
	Indicates the manufacturer's catalogue number
	Indicates the manufacturer's serial number so that a specific device can be identified
	Indicates the need for the user to consult the user manual
	Contents of the distribution packages are fragile therefore it shall be handled with care
	This is the correct upright position of the distribution packages for transport and/or storage
	Distribution packages shall not be rolled or turned over
	Distribution packages shall be kept away from rain and be kept in dry conditions

Sign	Description
	Distribution packages shall not be exposed to sunlight
	This Instrument is Subject to Laws Regarding the Disposal of Electronic Medical Equipment as Outlined in the WEEE Directive (2006/96/EC)
	Maximum number of identical transport packages/items which may be stacked on the bottom package, where "2" is the limiting number.
	Temperature limit(s)
	Humidity limit(s)
	FCC Compliant
	Medical Device
	Authorized representative in the European community/European Union
	Product complies with applicable European Union (EU) regulations


2. Use of Gelida 47

2.1 Product structure

2.1.1 Layout & Configurations

The hardware configurations of the Gelida 47 are shown in the figures below:

GELI-01-CE/US

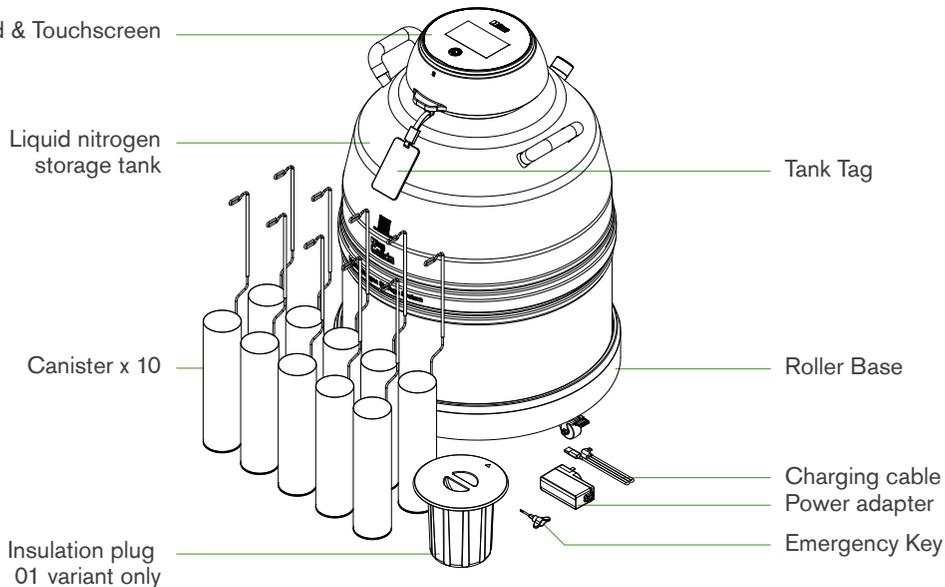

GELI-02-CE/US

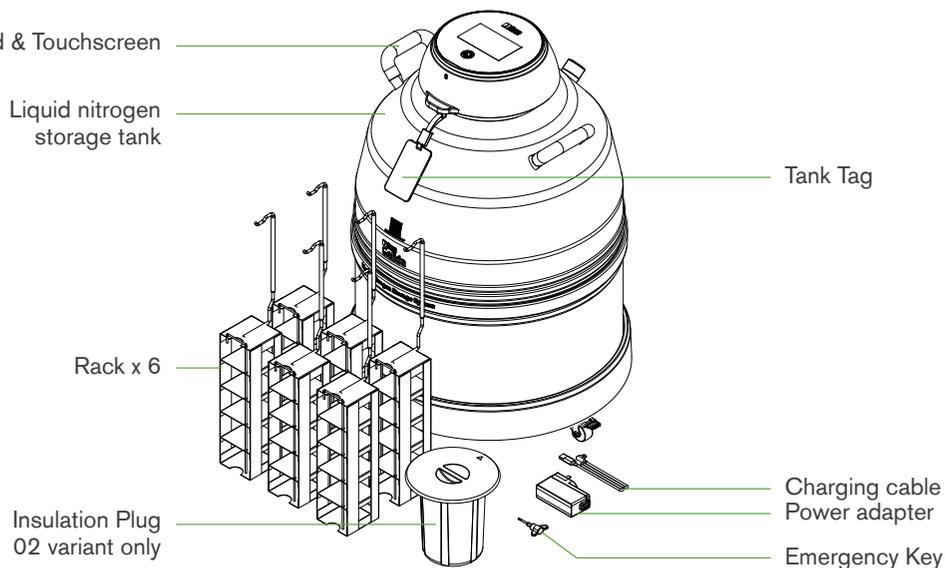


Figure 2-1 Basic Hardware Configuration (GELI-01-CE/US & GELI-02-CE/US)

The Gelida 47 composed of a smart lid and a tank, as shown in Figure 2-2:

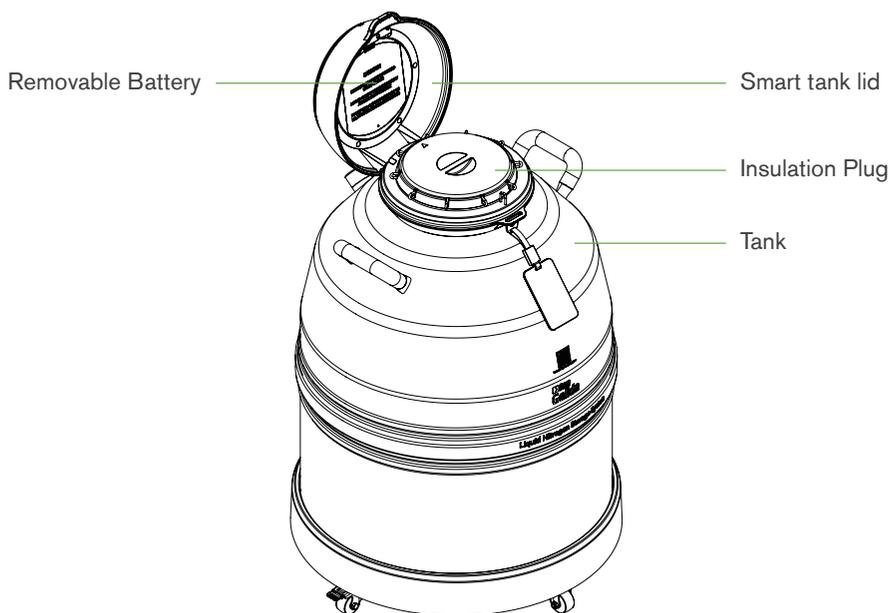


Figure 2-2 Configuration of the Liquid Nitrogen Storage Tank

a. Components of the tank lid:

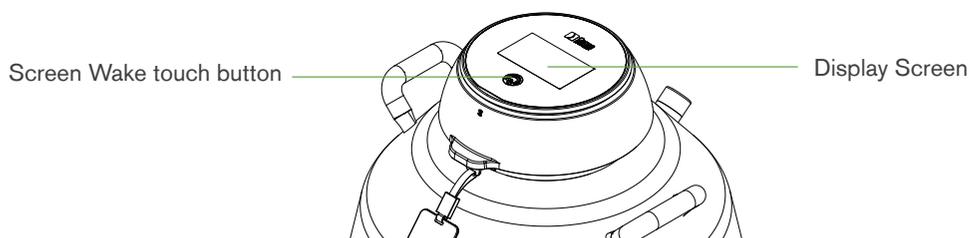


Figure 2-3 Tank Lid - Front View

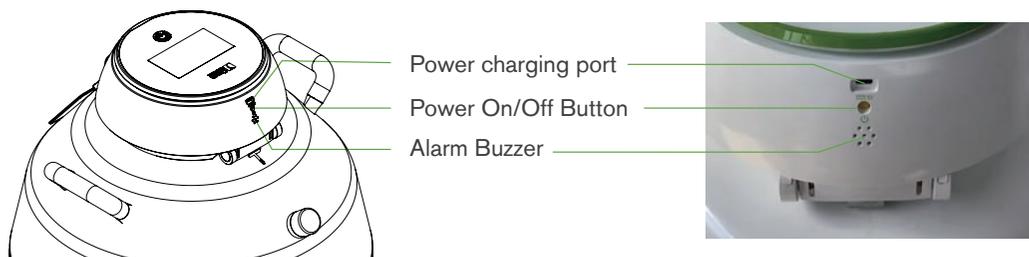


Figure 2-4 Tank Lid - Rear View

b. Tank and accessories:

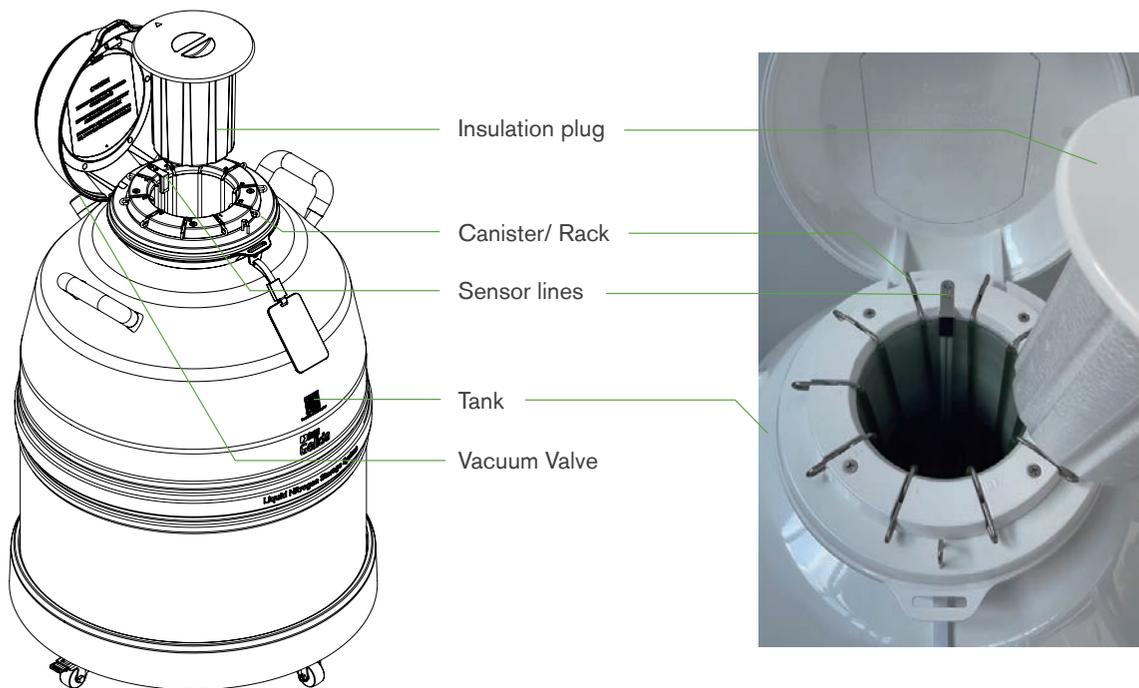


Figure 2-5 Tank and Accessories

	<p>CAUTION:</p> <p>The insulation plug, canisters and racks are not designed to be interchangeable between the canister and rack models (GELI-01-CE/US and GELI-02-CE/US, respectively). Do not mix and match canisters, racks or insulation plugs, use non approved components, or attempt to modify the device to accept non-approved components. Doing so may cause damage to the product, negatively impact product performance, cause malfunction of product features or void the product warranty.</p>
	<p>CAUTION:</p> <p>The vacuum valve is designed with a structure that allows for repeated air extraction. Tank vacuum maintenance should be carried out by the manufacturer or trained Genea Biomedx service representative. Customers are prohibited from attempting these procedures themselves to avoid negative impacts to the product's performance and avoid voiding warranty.</p>

2.2 Included accessories

2.2.1 Emergency Key

In the event of an emergency or an unlocking fault, the following symbol will be displayed in the centre of the display as shown below:



Figure 2-6 Lock Fault Icon

In this situation an emergency key is required to open the tank lid.

The steps are as follows:

- 1) Insert the key into the emergency key slot as shown in Figure 2-7.

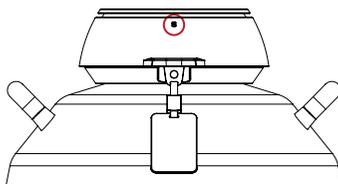


Figure 2-7 Emergency Key Slot

- 2) Align the key with the slot and turn it counterclockwise until it unlocks.

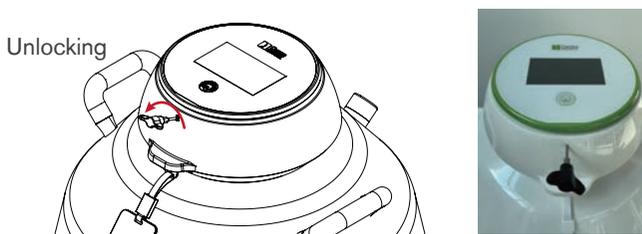


Figure 2-8 Unlocking Operation



NOTE:

The emergency key bypasses the digital logging and user password verification features; and retain a log of historical access when the manual emergency key is used to open the lid. If the lock is not functioning correctly, contact your authorized Genea Biomedx service representative to organise a repair or service visit.

2.2.2 Battery

The Gelida 47 comes with a removable and rechargeable lithium-ion battery. The battery consists of a charge status indicator light with LED indicating the current charge state, a battery on/off button for power safety protections.

To turn on the battery: Press the power on/off button on the side of the battery. The battery indicator lights will illuminate.

To turn off the battery: Press and hold the power on/off button on the side of the battery for more than 2 seconds. The indicator lights will turn off.

Battery indicator light: When the LED light is on and flashing rapidly, it indicates the battery is low and needs to be recharged and/or replaced (see Section 2.2.4). When charging, the Battery Indicator will flash slowly according to its charge state. When the battery is fully charged, the LED light is always on.

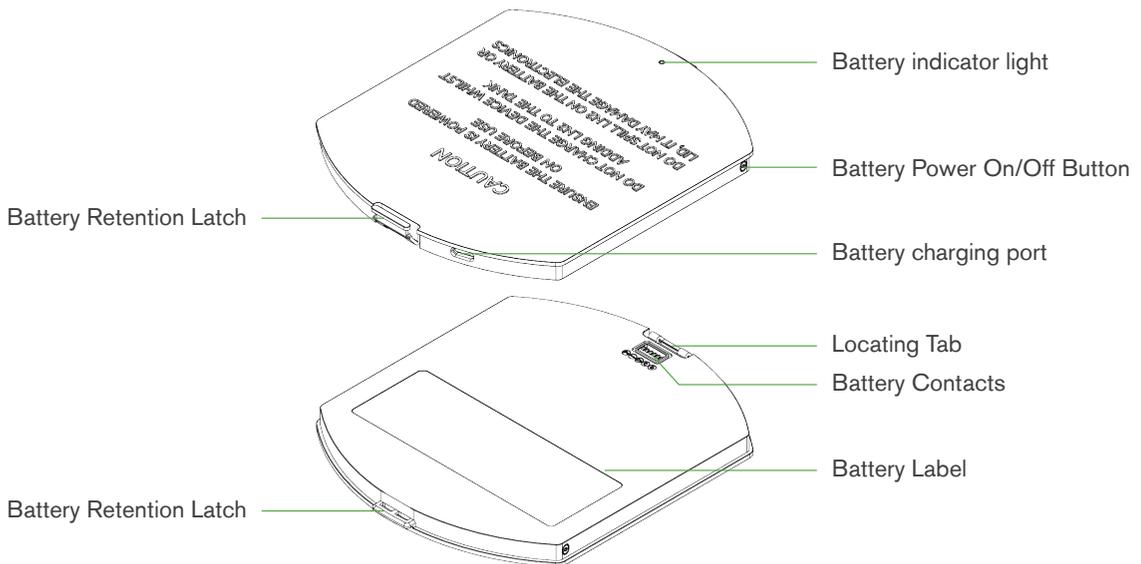


Figure 2-9 Battery



WARNING:

Misusing or mishandling the battery may result in fire or explosion. Only use the battery within the listed specifications provided with the battery pack.

Only use with the Gelida 47 and Battery with the approved charging accessories.

If the battery is visibly damaged or exhibiting signs of possible damage, please discontinue use immediately and contact your local Genea Biomedx representative.

2.2.3 Power supply

The tank can be connected to a 110-220V electrical supply via an external power adapter during operation. When the external power adapter is connected, the external power adapter supplies power to the device and charges the installed battery. When there is no external power adapter connected, the installed battery discharges and directly powers the device. A battery must be installed for the tank to work; the device will not be operable without a battery installed, even while plugged in to the power adapter.

2.2.4 Power adapter and charging cable

2.2.4.1 Charging

Connect the power adapter to the wall socket. Connect the charging cable to the power adapter and insert the USB-C end of the charging cable into the power charging port on the back of the lid (Figure 2-10). The lid should be powered on when charging. When charging, the battery icon will change to charging status.

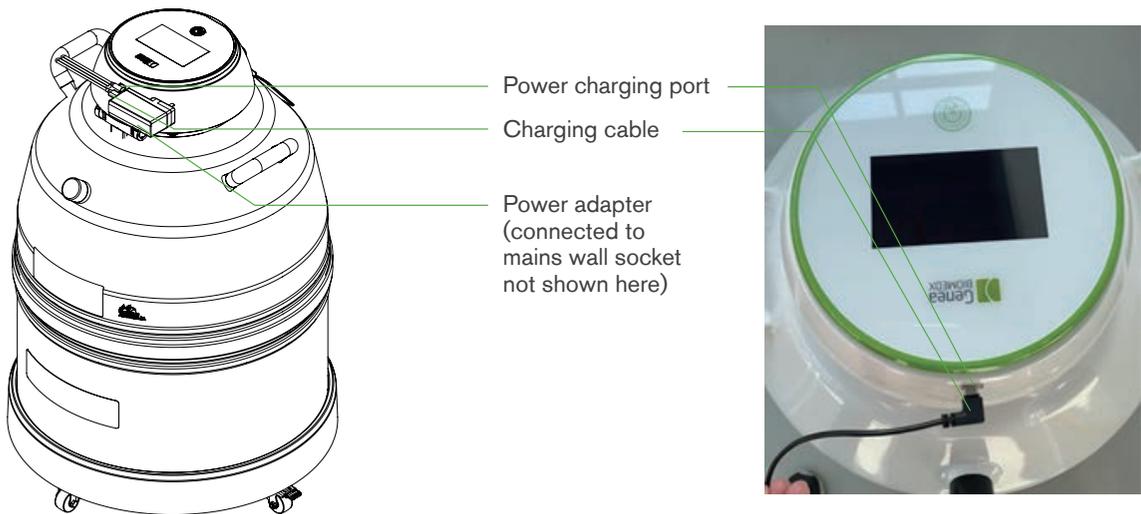


Figure 2-10 Charging Device



WARNING:

To reduce the risk of electric shock:

- Liquids, including liquid nitrogen, must not make contact with the tank lid or electronics; doing so may result in electrical short circuits.
- Do not replace the supplied charging power cord and/or power adapter with an incorrectly rated cord or adapter;
- Connect the charging power adapter only to an electrical power source with the proper voltage and frequency;
- Immediately replace the power cord if it becomes damaged, frayed, cracked or broken.

2.2.4.2 Replacing the battery

When the device is low on battery, the depleted battery can be replaced with a fully charged battery pack. The battery replacement touchpoints are indicated in Figure 2-11.

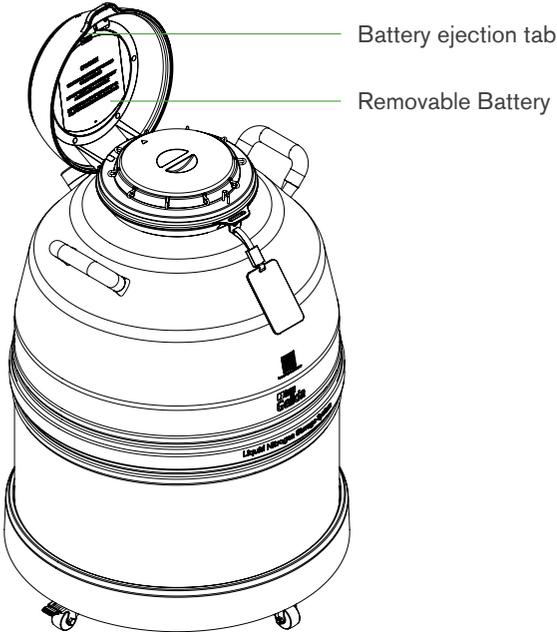


Figure 2-11 Battery removal and ejection touchpoints

To eject the battery: If the device is already powered and in use, unlock the lid with a valid username and password, and keep the lid in the open state. If the device is unpowered, you will need to use the emergency key to open the lid. Before removing the battery, press the power on/off on the back of the Gelida 47 Lid to power off the device (Figure 2-5). With the lid open, flex the Battery Retention Latch and remove the battery by hand (Figure 2-12, Steps 1,2 and 3).

To insert the battery: Check the battery power is on (Section 2.2.2) and has sufficient charge . Open the lid and put the new battery in place (Figure 2-12, Steps 4,5 and 6) taking care to align the locating tab on the rear of the battery into the locating slot correctly. Ensure the latch is fully engaged and that the battery is flush with the inner lid. Then close the lid. Press the power on/off on the back of the Gelida 47 Lid to power on the device. Confirm that the display wakes and the tank lock function are operating correctly.

	<p>NOTE: Perform battery replacement operations with care and ensure all retention mechanisms are correctly engaged.</p>
--	---

BATTERY EJECTION



BATTERY INSERTION



Figure 2-12 Battery replacement: Ejection (left 3 figures) and Insertion (right 3 figures)

2.2.5 Insulation plug

The insulation plug provides non-sealed insulation to maintain low temperatures within the tank, but allowing for gas to gradually escape as LN2 boils off. Correct installation of the insulation plug is as shown in the figure 2-13. The insulation plug should be positioned with the “Alignment Arrow” pointing vertically towards the hinge of the tank lid. The insulation plug should not require significant force to remove or reinsert. Ensure the cap is flush with the surface (not protruding) and rack/canister handles are correctly seated before closing the lid.

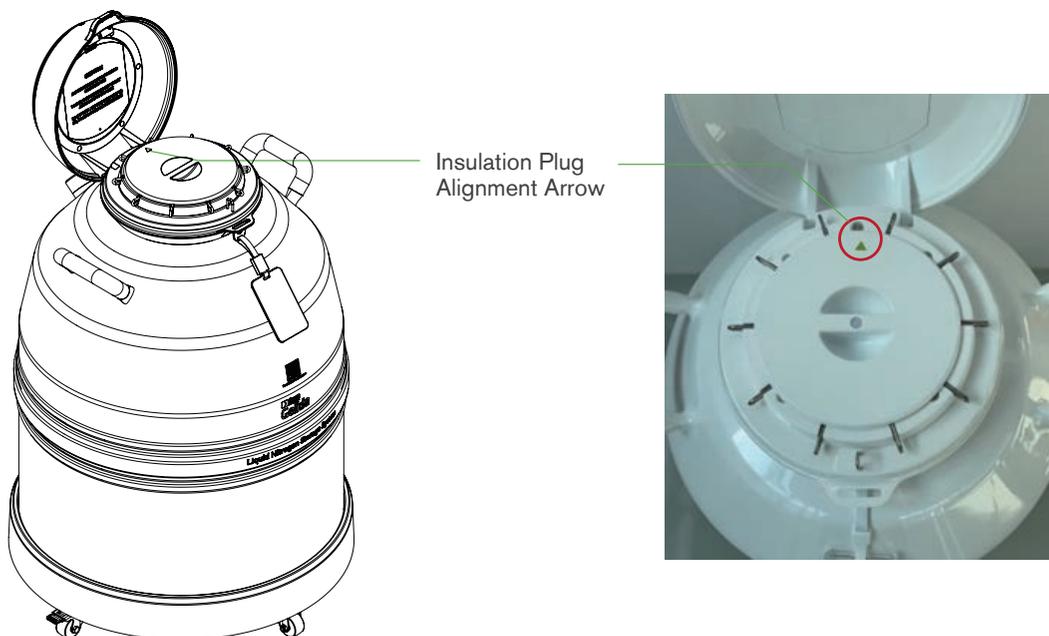


Figure 2-13 Insulation Plug Installation and correct orientation

	<p>CAUTION:</p> <p>Do not force the insulation plug into place. Do not modify the insulation plug in any way. Damage or modification to the insulation plug may result in degraded product safety and performance. If the insulation plug is damaged, excessive LN2 usage may occur, or in severe cases, excessive pressure may build up which could result in explosion. Transfer samples to a backup cryostorage solution and contact your local Genea Biomedx representative for support.</p>
	<p>NOTE:</p> <p>The insulation plugs are unique to each variant and are not interchangeable between the rack and canister models.</p>

2.3 Product setup & installation

The commissioning & installation of the product before first use should be done by a certified Genea Biomedx Field Service Engineer (FSE). The following instructions are guidance instructions which can be actioned by the customer after the FSE has installed the unit.

2.3.1 Installation space

Ensure the device is not placed in a location that makes it difficult to access, move, or open the lid.

Adequate space should be reserved around the device as shown in Figure 2-14 (units in mm). Ensure that there is sufficient space above the unit to allow users to open the lid, read the screen. Ensure there is some clearance on the sides of the tank where the handles are located so that the tank handles can be accessed, and to minimise risk of knocking into other tanks or objects.

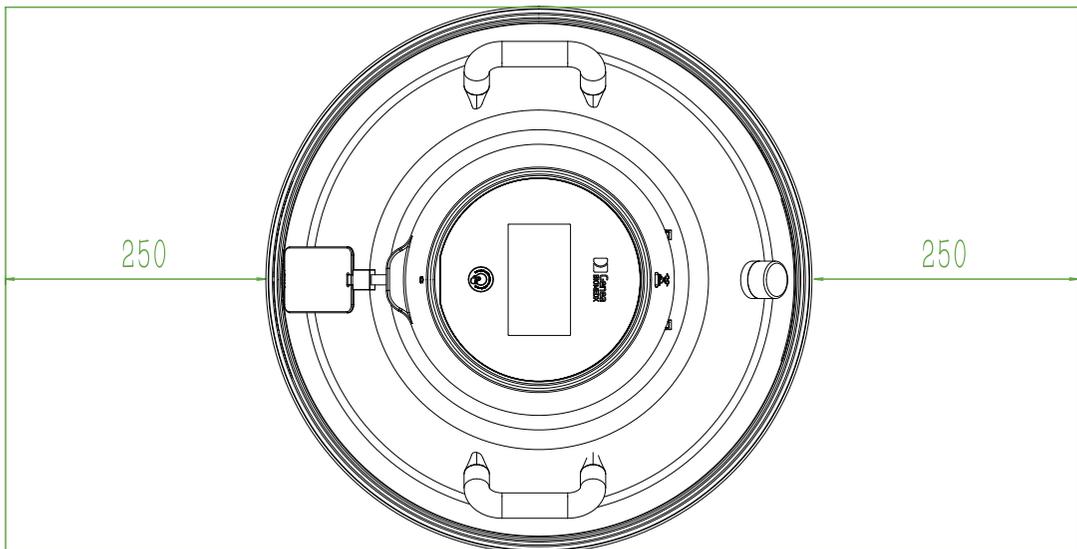


Figure 2-14 Minimum recommended spacing in front and behind tank (units in mm)

	<p>WARNING:</p> <p>Do not store or use container in areas that are small and enclosed or have poor ventilation. The venting of nitrogen gas may deplete oxygen in the air, possibly leading to asphyxiation or even death. It is recommended to add an oxygen concentration monitor and alarm in the tank room for additional user safety.</p>
	<p>WARNING:</p> <p>Do not tightly seal liquid nitrogen container or prevent nitrogen gas from escaping. Avoid excessive humidity levels or exposure to liquid ingress that could result in freezing of the insulation plug, and possible explosion.</p>

  	<p>CAUTION:</p> <p>Handle the cryopreservation vessel with care during use, failure to handle with care may impact the product safety and performance and may void warranty.</p> <ul style="list-style-type: none"> • Never overfill Gelida 47 with liquid nitrogen. Liquid nitrogen should always be below the bottom of the neck tube. Overfilling the tank may cause immediate or premature vacuum failure to occur. • Never ship Gelida 47 on its side or upside down. • Remove and insert inventories carefully. Do not scratch neck tube area. Scratches can cause premature vacuum failure. • Never tamper with or removing the vacuum port as this may result in vacuum failure. • Never drop or hit the unit. • Never spill liquid nitrogen on or near vacuum port. • Never leave the vessel in outdoor conditions. • Never place the unit near a heat source. • Never have items stacked on top of the product. • Performance data available for the instrument is based on static conditions only. Actual performance will vary upon the nature of use. Addition or removal of samples, addition on non-validated accessories, along with vibration will decrease the working duration of these products.
	<p>WARNING:</p> <p>Do not place or use instrument near a strong source of RF radiation (e.g., an unshielded radio frequency (RF) source). Doing so may interfere with the electronics and communication functionality of the instrument.</p>
	<p>NOTE:</p> <p>It is recommended to keep a spare tank filled with liquid nitrogen on hand for emergency should a tank in service become damaged or lose vacuum, enabling rapid transfer of samples to the spare tank.</p> <p>It is the customer's responsibility to ensure adequate safety procedures are in place to save the samples contained within the tank.</p>

2.3.2 Installation method

1. Remove the Gelida 47 from its packaging place it in the Roller Base and move it to the selected installation location.
2. Open the lid and install the removable battery follow the instructions as outlined in Section 2.2.2 to power on the battery and Section 2.2.4.2 to install.
 - a. Note: For the first installation, use the Emergency Key to open the lid.
 - b. Note: The device is not operable without a battery installed. Using non-approved batteries may result in device damage, and/or risk of explosion or fire.

3. Press the power on/off button to turn the device on.
4. The screen should automatically wake. If not, slightly touch the wake button on the tank lid to check if the screen can be normally awakened.
5. Connect the power adapter to the charging cable, then insert the cable into the power charging port to confirm normal charging.
 - a. Note: When charging, the battery icon will change to charging status. The charger can be removed once the battery is fully charged.


2.3.3 Opening the Tank Lid

1. Open the tank lid and lift the insulation plug.
 - a. If the lid is locked, wake the screen using the Wake Button on the lid, and follow the instructions in Section 2.4.6 to open the lid using the touch display.
 - b. If there is an unlocking failure, follow the instructions in Section 2.2.1 to use the Emergency key to bypass the electronic lock.
2. Remove any shipping packaging within the tank.
3. Confirm the presence of the canister/rack inside the Gelida 47 for every numbered location.

2.3.4 Filling Liquid Nitrogen

First Use:

1. Before initial use, check that the interior of the container is clean, dry and all packaging has been removed.
2. Open the tank lid. If the lid is locked follow the instruction in Section 2.4.6.
3. Carefully remove the insulation plug.
4. Fill with liquid nitrogen to required level. Adding liquid nitrogen to a warm container can cause significant boiling off and Nitrogen Gas. Fill slowly and gradually, some time may be required for the internal temperature to equilibrate.
5. After adding liquid nitrogen, install the rack or canister used for sample storage.
6. Re-insert the insulation plug and close the lid. Ensure the insulation plug is seated flush and in the correct orientation as in Section 2.2.5.
7. Visually inspect the tank after first fill for signs of vacuum loss, such as excessive frost or condensation on the outer shell of the tank. Minor frost at the top of filling is expected.
8. Perform touch operations on the display screen of the tank lid to set parameters, as detailed in Section 2.4.

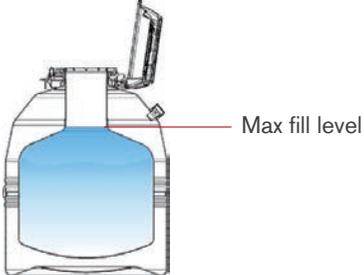	<p>WARNING:</p> <p>The Gelida 47 is exclusively designed to be used with liquid nitrogen ONLY and should not be used to store any other cryogenic substances.</p>
	<p>CAUTION:</p> <p>Never overfill vessels with liquid nitrogen. Liquid nitrogen should always be below the bottom of the neck tube (approximately 47.4L). Overfilling may cause immediate or premature vacuum failure to occur, and it may also cause spillage, which can damage the tank and the electronic components on the lid.</p> 
	<p>WARNING:</p> <p>Liquid nitrogen is extremely cold. To avoid injury by frostbite, use extreme care whenever handling liquid nitrogen, liquid nitrogen storage or transfer vessels, or any objects which have come in contact with liquid nitrogen.</p> <ul style="list-style-type: none"> • Appropriate cryogenic protective gear must be worn to prevent cryogenic burns; leave no areas of skin exposed. <ul style="list-style-type: none"> ◦ Safety attire over clothing ◦ Face shield ◦ Cryogenic gloves ◦ Cryogenic apron • Use extreme care to prevent spilling and splashing liquid nitrogen during transfer. • Always keep vessel in upright position. Do not tilt or lay the vessel on side. • Get immediate medical attention for any frostbite injuries due to liquid nitrogen. • Immediately remove any clothing or safety attire on which liquid nitrogen has spilled. • When refilling with liquid nitrogen, pre-cool the system with a small amount of liquid nitrogen before refilling. The refilling process should be gradual to avoid splashing and potential cryogenic burn related injuries. 
	<p>WARNING:</p> <p>To reduce the risk of electric shock:</p> <ul style="list-style-type: none"> • Liquids, including liquid nitrogen, must not make contact with the tank lid or electronics; doing so may result in electrical short circuits. • Do not attempt to repair or modify any part of the instrument.
	<p>NOTE:</p> <p>The full capacity of Gelida 47 tank is designed to accept up to ~47L of liquid nitrogen. The actual volume of LN2 required to fill the tank may vary this amount if the tank temperature has warmed sufficiently.</p>

2.4 User operation

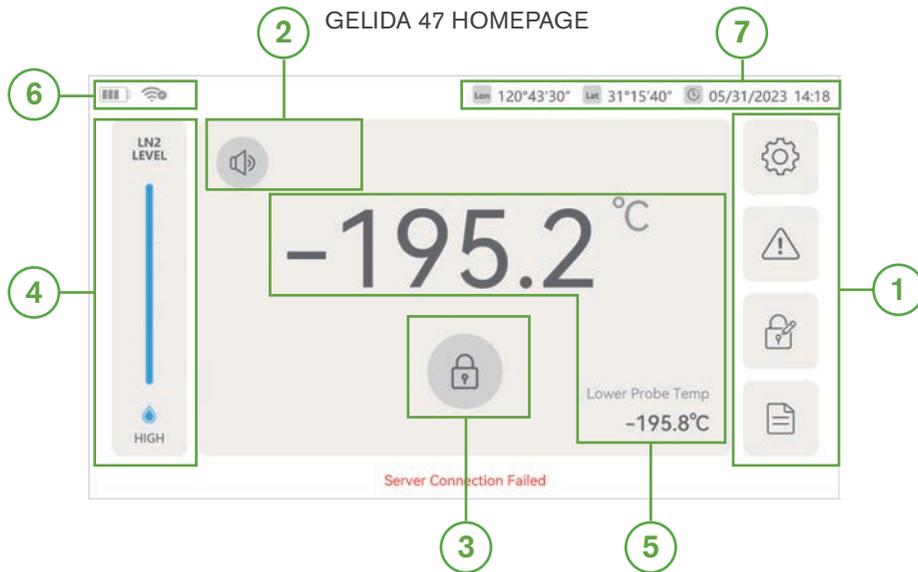


Figure 2-15 Homepage/Main Interface of Gelida 47 Display Screen

#	Description	Section Reference
1	Warnings	2.4.2
	Security	2.4.3
	Logs	2.4.4
	Settings	2.4.11
2	Alarm Mute Button	2.4.5
3	Lid Locking/Unlocking/Status Button	2.4.6
		2.4.7
4	LN2 Level Indicator	2.4.8
5	Temperature Display	2.4.9
6	Battery, Wi-Fi Status	2.4.10
		2.4.11.1
7	GPS Location and Time	2.4.11.2
		2.4.11.11

2.4.1 Turning on and using the Display

To turn on the touch display, tap the wake button on the lid. Ensure that the device is powered on.

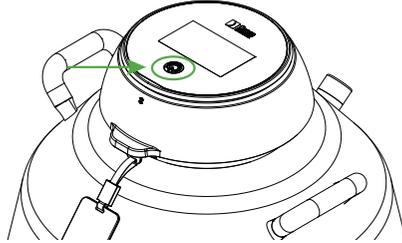


Figure 2-16 Screen wake touch sensitive button



NOTE:

The lid wake button and touch screen are capacitive. Touch functionality may be impacted by the type of gloves worn when using the touch features.

A slightly longer press may be required for the display elements to respond. Alternatively try touch functionality without using gloves or with alternative gloves if screen remains nonresponsive using existing PPE.

2.4.2 Warning & Faults Management

On the main interface, click on the "Warning" button to access the Warning & Fault records interface. Descriptions of Warnings & Faults can be viewed in Section 4.4.

Icon	Description
	No active warnings: Historical warnings and faults can be viewed
	Active Warning or Faults which require user intervention to resolve

If there are many warnings, the list will be distributed across multiple pages. The pages can be navigated by clicking on the and buttons on the lower bar of the display. The current page number is displayed in between the navigation arrows. Warnings & faults must be completely resolved before the Warning Indicator will reset.

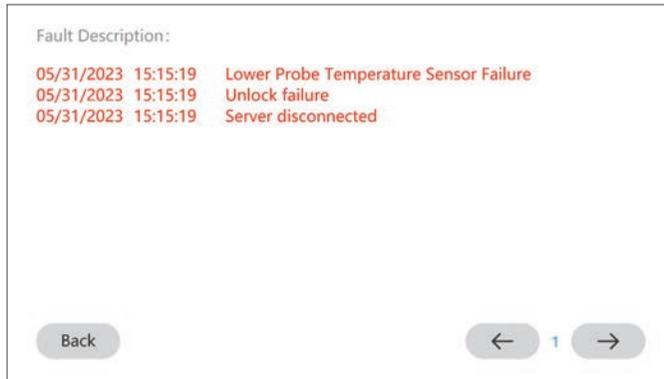


Figure 2-17 Fault Description

	<p>NOTE:</p> <p>A maximum of 100 of the most recent warnings or faults can be stored . If the tank is linked to a monitoring system, warnings and faults can also be viewed there.</p>
---	--

2.4.3 User Password Modification

To modify the password, click on the “Security” button on the homepage to navigate to the following interface.

Icon	Description
	Access the “Security” interface to modify user passwords

Enter the correct username and current password. If there is an error in the input, a red font warning will be displayed . Upon correct entry of the details, input the new password and confirm the password, ensuring both entries are identical. Click on "Confirm" to receive a prompt about the modification result. Once the prompt indicates successful modification, the new password can be used to log in.

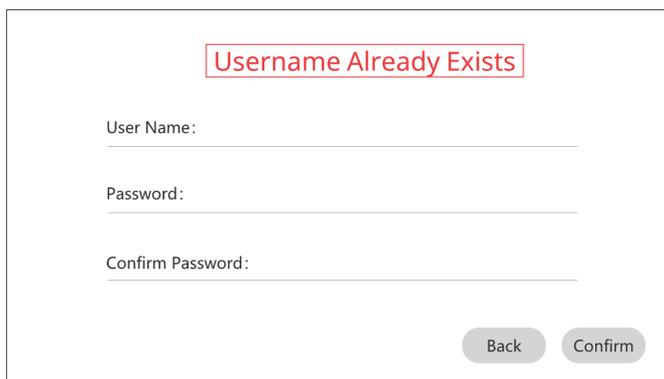


Figure 2-18 Password Modification Interface

2.4.4 System Access Logs

On the homepage, click on the button “System Access Logs”. A password prompt will appear as the detailed access and operational logs require the local administrator password for the Gelida 47 unit.

Icon	Description
	Access the “System Access logs” interface to see all records of tank access

For assistance with the Administrator password, refer to Section 2.4.11.4.

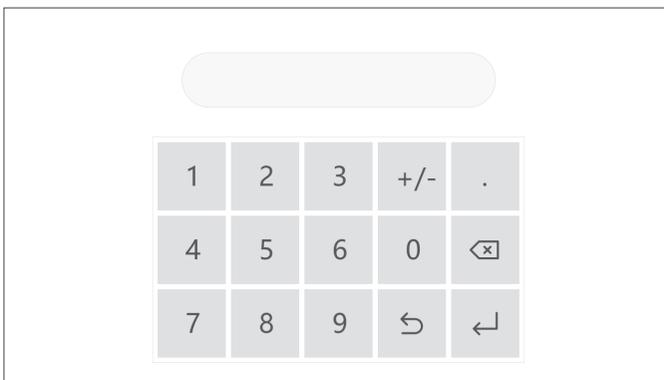


Figure 2-19 Password Input Interface

The Access Log Inquiry Interface indicates the time of the log event, the access event type, the user, and the witness. If there are many log entries, the list will be distributed across multiple pages. The pages can be navigated by clicking on the “arrow” buttons on the lower bar of the display. The current page number is displayed in between the navigation arrows. Click the “Back” button to go back to the Homescreen.

Operation Time	Event	Operator	Witness
05/31/2023 15:19:31	Lock		
05/31/2023 15:18:31	Unlock	001	
05/31/2023 15:16:20	Lock		
05/31/2023 15:15:19	Unlock	001	002

Back ← 1 →

Figure 2-20 Log Inquiry Interface

2.4.5 Alarms & Muting Alarms

The audible alarm will be triggered when an alarm condition is met which requires user intervention to resolve.

When the buzzer emits an alarm sound, the silence/mute button can be clicked to silence the sound, the icon's background colour changes to blue, and the alarm sound ceases. Ten minutes after clicking the mute button, the mute is released, and the alarm sounds again.

Icon	Status	Description
	Alarm On	If the icon appears like this, the alarm buzzer is on and will emit an audible sound in an alarm condition.
	Alarm Muted	The audible alarm is temporarily muted for 10 minutes. The button can be tapped again to un-mute the audible alarm at any time.

	<p>NOTE:</p> <p>Muting the alarm is temporary, the system will continue to alarm if the original cause is not addressed. To identify and address the alarm condition, referring to Warnings Module in section 2.4.2. If available and connected, the alarm condition can be communicated to some types of monitoring system if connected even when muted. Discuss with your local Genea Biomedx representative to see if connection to external monitoring solutions are available in your region.</p>
---	---

2.4.6 Lid operation

The Gelida 47 tank is equipped with a digitally controlled electromechanical lock with single or dual password authentication. The lock icon and statuses are located in the centre of the display as indicated in Figure 2-15 Icon 3.

Icon	Status
	<p>Lid Locked</p> <p>Tap this icon to enter credentials to unlock tank lid</p>
	<p>Lid Unlocked</p>
	<p>Lid Locking Fault</p> <p>Audible Alarm – Consult Section 4.4 for troubleshooting</p>
	<p>Lid Unlocking Fault</p> <p>Audible Alarm – Consult Section 4.4 for troubleshooting or use the emergency access key</p>

When the device has single-password verification enabled, the lid opening and closing operation is as follows:

2.4.6.1 Unlocking lid

Click on the lock icon (Icon 3 in Figure 2-15), enter the operator's username and password and press the "confirm" button. Upon successful entry, the lock opens, and the lock icon changes to lid unlocking status.

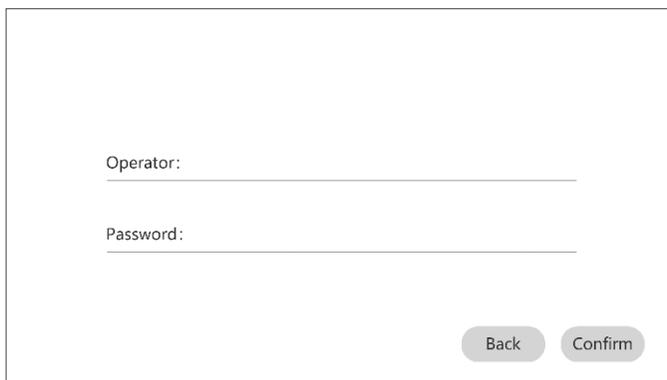
The image shows a user interface for entering a password. It consists of two text input fields. The first field is labeled "Operator:" and the second is labeled "Password:". Below the "Password:" field, there are two buttons: "Back" and "Confirm". The "Back" button is on the left and the "Confirm" button is on the right. Both buttons are rounded rectangles with a light gray background and dark text.

Figure 2-21 Unlocking Password Input Interface

2.4.6.2 Locking lid

Ensure the canisters or racks have been replaced are seated correctly, and the insulation plug has been correctly placed. Press to close the lid, the lid will be locked, and the lock icon changes to lid locking status.

In case of a fault, the lock icon remains unchanged, and the colour turns red, the alarm buzzer will emit an audible alarm, and a record is added to the Warnings & Faults log.

When the device has Dual Password Authentication enabled:

The lid opening and closing operation requires:

- 1) Operator username and password.
- 2) Witness username and password.

The lock will only open if both the operator's and witness's usernames and passwords are correctly entered.

Witness: _____

Password: _____

Back Confirm

Figure 2-22 Witness Login Interface

**NOTE:**

If the screen lights up and there is no operation for more than 3 minutes, the screen will automatically turn off and enter sleep mode, but electronic and monitoring components are still running internally.

To determine if the device has entered sleep mode by touching the screen. If the touch screen does not light up upon touch, it means that the device has entered sleep mode.

2.4.7 Sample access

2.4.7.1 Accessing a Canister/Rack & Sample

After opening the tank lid, carefully take out the insulation cap, and take out the canister/rack of choice. For ease of access and location tracking, the canister positions are numbered next to the locators as circled in Figure 2-23.

Lift the desired canister or rack by the handle which is hooked on the neck of the lid. Ensure that your approved lab procedure is followed when handling all cryogenically stored samples.

Add or remove the required sample(s) and return the canister or rack to the original position. The position is indicated on the plastic rim of the lid.

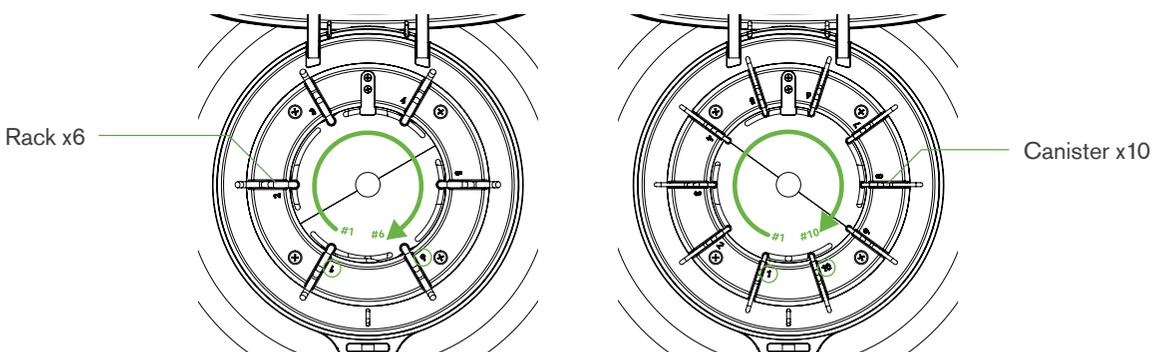


Figure 2-23 Numbered positions of canisters and racks

	<p>NOTE:</p> <p>Additional coloured indicators and/or labels can be added to the canister and rack handle(s) to provide additional information or enhance ease of identification. Ensure that any additional indicators do not interfere with the lid closure/locking, insulation cap positioning or handle notches for canisters/racks.</p> <p>Consult with your local Genea Biomedx representative for more information.</p>
---	---

2.4.7.2 Replacing a Canister/Rack & Sample

Before closing the lid, replace the sample into the canister or rack, and ensuring that it cannot fall out. For the Rack variant, ensure that the retaining bar which holds the boxes in place.

Carefully lower the canister or rack into the tank, being careful not to damage or scratch the internal structure of the tank. Check that the canister or rack is returned to the correct position it was removed from.

Ensure the handle is correctly engaged with the correct position in the lid, and carefully replace the insulation cap.

	<p>WARNING:</p> <p>Liquid nitrogen is extremely cold. To avoid injury by frostbite, use extreme care whenever handling liquid nitrogen, liquid nitrogen storage or transfer vessels, or any objects which have come in contact with liquid nitrogen.</p> <ul style="list-style-type: none"> • Appropriate cryogenic protective gear must be worn to prevent cryogenic burns; leave no areas of skin exposed. <ul style="list-style-type: none"> ◦ Safety attire over clothing ◦ Face shield ◦ Cryogenic gloves ◦ Cryogenic apron • Use extreme care to prevent spilling and splashing liquid nitrogen during transfer. • Always keep vessel in upright position. Do not tilt or lay the vessel on side. • Get immediate medical attention for any frostbite injuries due to liquid nitrogen. • Immediately remove any clothing or safety attire on which liquid nitrogen has spilled. • When refilling with liquid nitrogen, pre-cool the system with a small amount of liquid nitrogen before refilling. The refilling process should be gradual to avoid splashing and potential cryogenic burn related injuries.
	<p>CAUTION:</p> <p>When accessing frozen samples work quickly and carefully to avoid premature thawing and unnecessary sample loss.</p>

2.4.8 LN2 Liquid Level Estimate

The Gelida 47 has two temperature sensors that allow for estimation of LN2 liquid level. The upper temperature sensor and the lower sensor are located 21.6cm (8.5”) and 7.1cm (2.8”) from the tank bottom respectively. As the LN2 liquid level reduces, the liquid level will pass the temperature sensor resulting in an increase in measured temperature. The monitoring system interprets the temperature differential between the top and bottom sensors based on the set limits, and displays an estimate as High, Medium or Low.

Icon	Meaning	Approx. LN2 Volume*
	Homescreen display shows an estimate for the current liquid level determined from the temperature of the upper and lower tank temperature sensors. The LN2 level estimate can be high, medium, or low, with the current estimate coloured, and non-active levels in grey.	-
	The display is blue and the LN2 level is estimated to be high.	34L – 47L
	The display is orange and the LN2 level is estimated to be between high and low: replenish, or plan to replenish LN2 soon.	14L – 34L
	The display is red and the LN2 level is estimated to be low, immediately replenish LN2 to protect stored samples.	< 14L

*Note: Values based on upper and lower temperature sensor limits set to -195°C as shown in the table below. It is recommended to validate the levels according to your internal risk profile for the samples to be stored.

The table below indicates the expected liquid level estimation behaviour with the upper and lower temperature sensor limits set to -195°C. It is recommended to validate the temperature sensor limits and liquid level estimation according to the use case. Alarm temperature limits can also be set by the user (see Section 2.4.11.6 & 2.4.11.7).

Displayed Estimate	Upper Temperature Sensor Reading	Lower Temperature Sensor Reading
High Liquid Level	≤ -195°C	≤ -195 °C
Medium Liquid Level	> -195°C	≤ -195 °C
Low Liquid Level	> -195°C	> -195°C

	<p>WARNING:</p> <p>Never use a hollow tube to measure liquid nitrogen level. This could lead to thermal injury. The device is equipped with 2 temperature sensors which are used to approximate the liquid level in the tank.</p> <p>Contact local your Genea Biomedx representative if you need alternative methods to measure liquid nitrogen level.</p>
	<p>NOTE:</p> <p>Upon powering on the device, it's normal for the liquid level icon to appear grey as data is being acquired and refreshed.</p> <p>When either the high or low temperature sensors experience a fault, all liquid level icons will remain grey. Contact your authorised Genea Biomedx Service representative immediately for servicing.</p>

2.4.9 Temperature Display

The temperature displayed in the centre of the Homescreen is the reading from the “Upper Probe Temperature Sensor” (Figure 2-24 A). The “Lower Probe Temperature” displays the reading from the “Lower Probe Temperature Sensor” (Figure 2-24 B).

When the temperature of either sensor exceeds the set limit, the temperature reading will change from grey to red , and an alarm will sound.

If the tank is linked to a monitoring system, an alarm notification will also be sent.

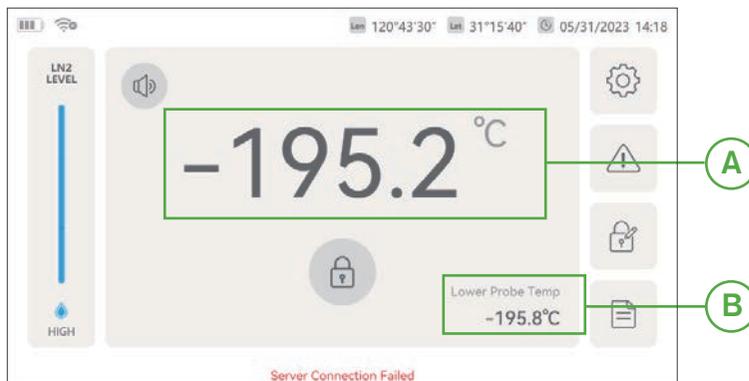


Figure 2-24 Upper (A) and Lower (B) Temperature Probe readings displayed on the user interface

2.4.10 Battery Level Display

The battery level of the tank lid is displayed in the upper left corner of the Homescreen. There are five states of battery level, and any abnormalities are coloured.

Icon	Description
	The battery icon shows 4 grey bars; the battery level is indicated between 75% and 100%.
	The battery icon shows 3 grey bars; the battery level is indicated between 50% and 75%.
	The battery icon shows 2 yellow bars; the battery level is indicated between 25% and 50%.
	The battery icon shows a single red bar; the battery level is indicated less than 25%. Note: When the icon is flashing, it indicates the battery level is extremely low and needs to be urgently recharged and/or swapped for a fully charged battery
	The battery icon shows a green power symbol; this indicates that the battery is being charged.

2.4.11 Settings

Click on the “Settings” button. Modification of settings requires the administrator password. The default administrator password can be found in Section 2.4.11.4.

Icon	Description
	Access the “Settings” interface for the tank

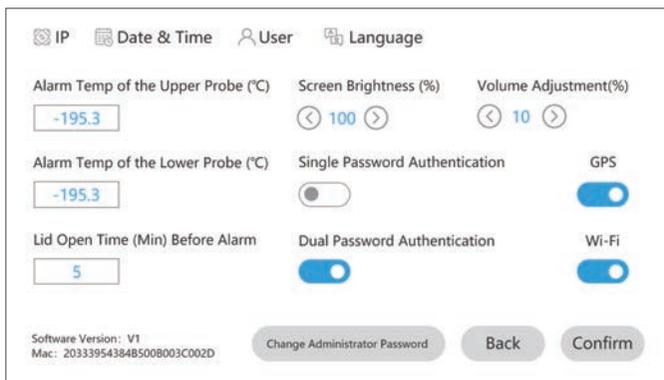


Figure 2-25 Settings Interface

2.4.11.1 Wi-Fi & IP settings

The device Wi-Fi must be enabled to connect to the Gelida 47 Tank to the monitoring systems. The monitoring system allows for additional functionality with the Gelida 47 tank and Gelida Ecosystem, such as remote tank monitoring, alarms, notification, permissions management and additional sample management.

To enable connection to the Monitoring system, contact your local Biomedx Representative for more information.

IP Setting steps:

- 1) Tap the IP button in the Setting Interface;
- 2) The IP Settings page will appear as in Figure 2-26;
- 3) Select Monitoring system IP, and enter the server:
 - a. IP address
 - b. Server Port
 - c. Wi-Fi SSID
 - d. Wi-Fi Password
- 4) Review details and click "Confirm".

The screenshot shows a settings screen with the following fields and buttons:

- Local IP: _____
- Server IP: _____
- Server Port: _____
- SSID: _____
- Password: _____
- Back (button)
- Confirm (button)

Figure 2-26 IP Settings

	<p>NOTE:</p> <p>The Monitoring system & Gelida 47 Tank must be on the same local network or virtual network to ensure a stable connection. Contact your local Biomedx representative for more information or for setup assistance.</p>
	<p>CAUTION:</p> <p>Do not place or use instrument near a strong source of RF radiation (e.g., an unshielded radio frequency (RF) source). Doing so may interfere with the electronics and communication functionality of the instrument.</p>

2.4.11.2 Date & Time Setup

To set the date and time of the internal clock on the Gelida 47, tap the Date & time button in the top bar of the setting screen. Click on the button, input the date and time, then click "Confirm".

The date format: MM / DD / YYYY (numerical)

The time format: HH: MM: SS (24 hour time)

The screenshot shows a 'Time Calibration' screen with two input fields. The first field is labeled 'Date:' and contains the text '05 / 31 / 2023'. The second field is labeled 'Time:' and contains the text '14 : 26 : 09'. At the bottom right of the screen, there are two buttons: 'Back' and 'Confirm'.

Figure 2-27 Time Calibration

2.4.11.3 User management

After tapping the "User" button on the Setting interface, users can enter the user management page.

The lower bar is the functional zone which allows for user profile management and contains the "Create User" and "Delete User" buttons, as well as page navigation arrows. The upper part is a table which displays currently registered users and information, such as User "Serial Number", "User Name" and "User Creation Time".

User Serial number is automatically sorted by creation time. If there are many authorised users, the list will be distributed across multiple pages. The pages can be navigated by clicking on the ← and → buttons on the lower bar of the display. The current page number is displayed in between the navigation arrows.

Serial Number	User Name	Creation Time
1	006	05/31/2023 14:26:09
2	008	05/31/2023 14:02:57

At the bottom of the screen, there is a navigation bar with the following elements from left to right: a 'Create User' button, a 'Delete User' button, a left arrow button, the number '1', a right arrow button, and a 'Back' button.

Figure 2-28 User Management Interface

The following table outlines the 3 different authorization permissions on the Gelida 47 Tank, and the functions of each permission.

Functions	No Login	Operator	Administrator
Access information such as temperature readings, GPS location, time, Wi-Fi connection status	✓	✓	✓
View Warnings, Faults and Mute Alarm	✓	✓	✓
Open Tank Lid	✗	✓	✗
Enter and edit the device settings	✗	✗	✓
Create and Modify Users & Password	✗	✗	✓
View and clear Access Logs	✗	✗	✓

a) Create user


Click on the "Create User" button in user management to navigate to Figure 2-29.

- 1) Enter the User Name (three-digit numerical code).
- 2) Enter the User Passcode (numeric only and must be 6 digits long).
- 3) Re-enter to confirm Passcode.

Note: The passcode and confirm passcode must match; if they do not, a red font warning will appear on the interface.

- 4) Click "Confirm". If the user creation was successful, the new user will appear on the list in the user management interface.

Note: There is a maximum of 100 users (001-100), not including the administrator account. If the range is exceeded, a "Username must be 001 to 100" prompt will appear.

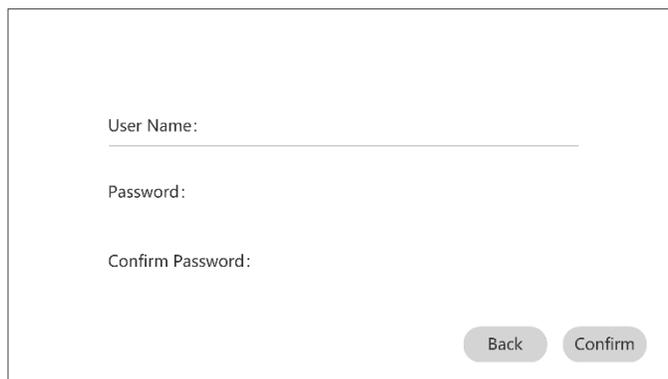

The screenshot shows a simple form with three input fields stacked vertically. The first field is labeled 'User Name:' and has a horizontal line for text entry. The second field is labeled 'Password:' and the third is labeled 'Confirm Password:'. At the bottom right of the form, there are two rounded rectangular buttons: 'Back' and 'Confirm'.

Figure 2-29 Create User Interface

b) Delete user

Click on the "Delete User" button in user management, which redirects to Figure 2-30.

Enter the "User name" of the user to be deleted. If the entered username is incorrect, a red font warning will appear on the interface; clicking "Delete" will proceed to delete the user, and they will no longer appear in the user management interface.

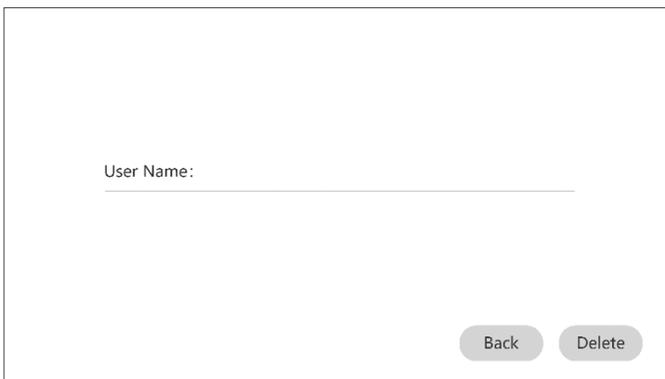
The screenshot shows a simple web interface for deleting a user. It features a text input field with the label "User Name:" positioned above it. Below the input field, there are two buttons: "Back" and "Delete", both rendered in a light gray, rounded rectangular style.

Figure 2-30 Delete User Interface



NOTE:

If the Gelida 47 Tank is connected to a monitoring system, it is recommended not to create or delete users on the Gelida 47 only.

Contact your local Biomedx representative for more information or for setup assistance.

2.4.11.4 Administrator password modification

The default administrator account allows for advanced access to key settings and user administration. By default, the administrator password is: 777777. To update the password, select the "Change Administrator Password". Enter the new password and confirm new password and click "Confirm". The password is numeric only and must be 6 digits long. If the " Configuration Successful" appears on the screen, it indicates that the password has been successfully reset.

New Password: _____

Confirm New Password: _____

Back Confirm

Figure 2-31 Administrator Password Modification

**NOTE:**

It is recommended to change the administrator password for security of access and to prevent undesired access or tampering with the system.

Do not forget the administrator password once it has been changed. In the case of a forgotten administrator password, contact your local Genea Biomedx representative.

For assistance with the Administrator password, refer to Section 2.4.11.4.

2.4.11.5 Language

Select the Language to switch the device language: When the background colour of the Chinese icon is blue and English is white, it means that the current language is Chinese; when the background colour of the Chinese icon is white and English is blue, it means that the current language is English.

Chinese English

Back Confirm

Figure 2-32 Language Setting Interface

2.4.11.6 Alarm Temp of the Upper Probe (°C)

Set the upper temperature limit for the upper part of the Gelida 47: When the temperature in the upper part exceeds this limit, an audible alarm will be triggered, the temperature display shifts to red, and an additional anomaly record is logged.

2.4.11.7 Alarm Temp of the Lower Probe (°C)

Set the upper temperature limit for the lower part of the Gelida 47: When the temperature in the lower part exceeds this limit, an audible alarm will be triggered, the temperature display shifts to red, and an additional anomaly record is logged.

2.4.11.8 Lid Open Time (Min) Before Alarm

Sets the maximum duration (in minutes) allowable for the lid to remain open on the tank. If the lid is opened for too long or forgotten to be closed, the buzzer will send out an audible alarm and logged. The maximum allowable value is 30 minutes.

2.4.11.9 Screen brightness (%)

Set the screen brightness, value: 10-100. The higher the value, the brighter the screen.

2.4.11.10 Volume Adjustment (%)

Set the volume of audible alarms, value: 0-100. The higher the value, the louder the alarm volume.

2.4.11.11 GPS Location

The GPS function is designed to assist in tracking and geo-locating the tank.

Icon	Description
GPS 	GPS functionality is disabled GPS is disabled No GPS co-ordinates will be displayed on the Homescreen
GPS 	GPS functionality is enabled
Lon 120°43'30" Lat 31°15'40"	GPS co-ordinates on Homescreen: shown as Longitude (E) and Latitude (N) in DMS (Degrees, Minutes, Seconds)
Lon --°--'--" Lat --°--'--"	GPS is turned on, and no GPS co-ordinates can be calculated

To enable GPS, enter the settings interface. Tap the "GPS" button. When activated, the background colour of the button turns from white to blue. When deactivated the button will turn from blue to white. To lock in the change, click the "Confirm" button.

After clicking the "Return" button and a waiting period of 2-3 minutes, the device's current longitude (E)

and latitude (N) in DMS can be viewed in the upper right corner of the main interface, indicating the devices current position.

If the tank is placed somewhere with a weak GPS signal or interference, the tank may not reliably be able to determine the GPS co-ordinates.

	<p>NOTE: GPS Functionality is not available in all regions and may not be available on your specific model. Please contact your local Genea Biomedx representative for more information.</p>
	<p>CAUTION: Do not place or use instrument near a strong source of RF radiation (e.g., an unshielded radio frequency (RF) source). Doing so may interfere with the electronics and communication functionality of the instrument.</p>

2.4.11.12 Wi-Fi toggle

Enable or disable Wi-Fi and interact with an external monitoring system. An external monitoring system can provide centralised monitoring, remote alarms and sample tracking for one or more Gelida 47 tanks and it is sold separately. Connection and setup to external monitoring system(s) should be completed by a qualified Genea Biomedx service representative. For Genea Biomedx supplied monitoring systems, refer to the monitoring system user manual.

Icon	Description	Icon	Description
	Wi-Fi is disabled		Wi-Fi is disabled or not connected
	Wi-Fi is enabled		Wi-Fi is enabled and connected

Within Settings, if the Wi-Fi is disabled or not connected, the button will display as red. Upon clicking "Confirm" button, the Wi-Fi icon shifts from red to grey when the connection is successfully established.

The table below outlines faults which may appear on the Homescreen display:

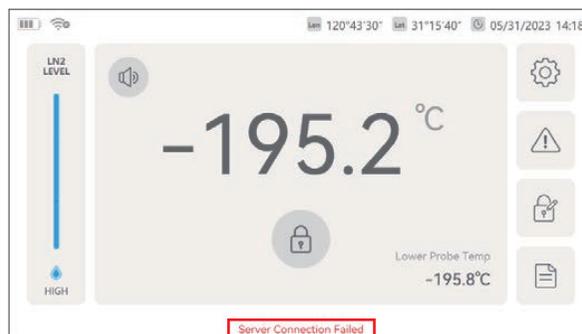


Figure 2-33 Error messages are displayed at the bottom of the Homescreen


The table below outlines faults which may appear on the Homescreen display:

Fault Display	Description
Router Connection Failed	The Wi-Fi SSID or password parameters in the IP settings are incorrectly set. Triggers Alarm.
Server Connection Failed	Initial connection to the monitoring system has failed, and a record is added to the exception record. Triggers Alarm.
Server Disconnected	A previously stable connection to the monitoring system was interrupted or disconnected for <2 seconds. No Alarm.

In all cases, a record of the exception is logged and can be reviewed in “Warnings and Faults” (Section 2.4.2).

2.4.11.13 Single/dual password verification

All Gelida 47 unlocking operations require password verification, which can be either single-password or dual password Authentication. There must be a minimum of two users created in the system for dual password verification to function. Refer to Section 2.4.12 on how to create additional users.

Operation Mode	Icon Display	Description
Single Password Verification		Single-password verification requires the correct entry of one operator’s username and password to open the tank.
Dual Password Authentication		Dual Password Authentication requires the correct entry of both an operator's and witness's usernames and passwords to open the tank.

Note: Selecting one verification mode, automatically disables the other option.

2.4.12 “Find My Tank” Function

Where the tank is connected to a compatible external monitoring system, the Find My Tank feature may be used. This feature allows for the tank to emit an audible and visual cue so that a tank may be quickly found in rooms where there may be many stored tanks.

When the device is in the "Find Tank" condition, the screen will display an icon accompanied by an audible alarm, and the screen stays on.

To stop the alarm, click on the “Find My Tank” icon; the audible alarm stops, and the icon disappears.

Icon	Description
	“Find My Tank” is currently active and an audible alarm is emitted

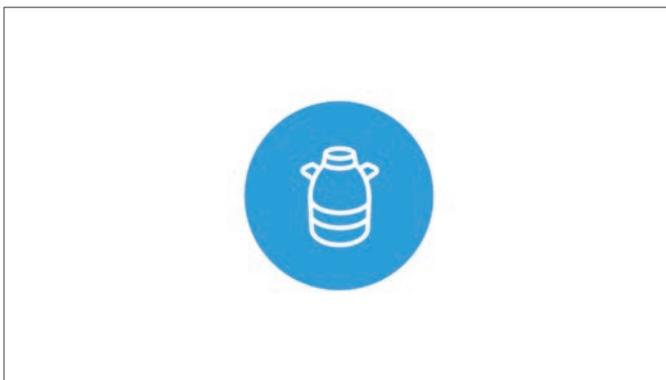


Figure 2-34 "Find My Tank" Interface



NOTE:

Frequent use of the “Find My Tank” function may drain the battery more rapidly.

3. Technical Specifications

Product Specifications	
Effective volume (L)	47.4±2.3L
Liquid nitrogen consumption	≤ 0.7 L/day Consumption may vary depending on storage conditions and frequency of tank opening.
Temperature detection error (°C)	At -196°C, the error is ≤±1°C
Battery life	Nominally 10 days
Packaging dimensions (mm)	600 × 600 × 930 (Length x Width x Height)
Device dimensions (mm)	540 × 540 × 805 (Length x Width x Height)
Net weight (kg)	30.3±3 kg
Approximate weight when full of LN2	68.7 kg
Canister Dimensions (mm)	278 x 72 (L x Diameter)
Maximum Box size for Rack (mm)	78 x 78 x 59 (Depth x Width x Height) – 5 boxes per rack
Mobility	Included 4-wheel roller base with 2 lockable feet
Service Life	5 years – extendable with repairs and maintenance
Operational Specifications	
Usage environment	Usage site: well-ventilated indoor area. Altitude: Below 2,000 meters. Environmental temperature: 5°C to 40°C. Environmental humidity: 20%RH to 80%RH, non-condensing.
Storage environment	Environmental temperature: 5°C to 40°C. Environmental humidity: 20%RH to 80%RH, non-condensing
Other Requirements	The product must always be kept upright, handled gently, and not tilted, laid horizontally, inverted, compressed, struck with other items, or subjected to impact.
Liquid ingress protection rating	IPX0
Operation Mode	Continuous Operation
Installation Type (Permanent or Non-Permanent)	Non-permanent installation / Mobile

Electrical Specifications & Standards

Power Adapter	Input: 100-240V~, 50/60Hz, 0.5A Output:5.0V 3.0A, 15.0W
Device Charging Port	Input: 5.0V $\overline{=}$ 3A Connector: USB Type C
Removable Battery	Model: GELI-BAT-01 Input:5.0V $\overline{=}$ 2A Output: 5.0V $\overline{=}$ 2A Rated Battery Capacity: 9.5 Ah / 35.15 Wh Battery Type: Lithium Polymer Battery
MCU model	STM32L431VCT6
Display Type	5.0-inch colour 1280 × 720 capacitive multi touch
Alarm Type	Audible Speaker 87±3dB – Single Tone Continuous Beeping
Electrical Safety	EN 61010-1:2010+A1:2019 Safety requirements for electrical equipment for measurement, control, and laboratory use -- Part 1: General requirements. IEC 61010-1:2010+AMD1:2016 Safety requirements for electrical equipment for measurement, control, and laboratory use -- Part 1: General requirements.
Electromagnetic Compatibility	EN IEC 61326-1:2021 Electrical equipment for measurement, control and laboratory use - EMC requirements -- Part 1: General requirements.

Network Connectivity Specifications

Network Connectivity	Wireless 802.11b/g/n
Network architecture	Client-Server (C/S)
Network bandwidth	No less than 10Mbit/s
Network type	LAN
Communications Protocol	TCP/IP protocol over a wireless network connection
Network security feature configuration	No external interfaces are available. Remote access control is disabled, and no configuration is required.
Data Encryption	Private protocol

Software & Security Specifications

Essential software	N/A
External software environment and security software updates	Not User Serviceable – trained field service engineer only
Ready-made software list	N/A
Security software compatibility list	No security software applicable
Data backup and disaster recovery	Not applicable
Connectable Software	Contact your local Genea Biomedx representative about connectable software options.

4. Product Maintenance & Support

4.1 Product Service Life

The expected service life of the Gelida 47 tank is 5 years. The products usable life may be extended through routine maintenance & calibration, preventative maintenance or service plans.

4.2 Routine maintenance & calibration

Periodic preventative maintenance and calibration should only be performed by personnel specifically trained by the manufacturer, such as a qualified Genea Biomedx service engineer.

4.2.1 Temperature Calibration

It is recommended that tank temperature sensor calibration should be conducted once a year. Schedule in annual calibration with your authorised Genea Biomedx Service representative.

4.2.2 Defrosting the Tank

Liquid nitrogen storage systems can have ice and frost build up over time if the lid is left open for prolonged periods or if the liquid level gets too close to the underside of the lid. Contact your authorised Genea Biomedx Service representative for guidance on frost removal.



WARNING:

Do not remove frost with hard objects to prevent further damage to the tank.

4.2.3 Tank Inspection & Monitoring

If a sudden increase in LN2 evaporation loss is found, or if excessive frost & condensation appears on the exterior surface of the Gelida 47, this may indicate tank damage or loss of tank vacuum. Ensure that tanks are inspected by operators on a regular schedule according to your lab protocol and risk management. Minor frost at the top of after filling is expected.

In such cases stop using the product immediately and contact local Genea Biomedx service representative. If samples are stored within the tank, carefully and quickly move them to alternative cryogenic storage.



CAUTION:

Tank vacuum maintenance and repair should be carried out by the manufacturer or trained Genea Biomedx service representative.

Customers are prohibited from attempting these procedures themselves to avoid negative impacts to the product's performance and avoid voiding warranty.

4.2.4 Decontamination

For cleaning, only the exterior of the tank should be cleaned using a clean dust-free cloth moistened with 75% alcohol, gently clean the tank lid and the exterior of the Gelida 47. The interior of the tank should only be cleaned by a trained Genea Biomedx service representative. Interior tank cleaning requires removal of all LN2 and samples to complete.

	<p>WARNING:</p> <p>Only authorised service personal should calibrate, repair or replace parts within the Gelida 47 or perform other service and repair activities.</p> <p>Attempting untrained repair may result personal injury, loss product features and performance, or voiding of product warranty.</p>
	<p>WARNING:</p> <p>To reduce the risk of electric shock:</p> <ul style="list-style-type: none"> • Do not attempt to repair or modify any part of the instrument; • Do not remove any of the instrument panels or covers.

4.3 Device Disposal

At the end of the product life, do not dispose of the tank with normal waste.

The tank is made from high quality aluminium alloy . The canisters and racks are constructed with stainless steel. The smart lid is comprised of moulded thermoplastic and incorporates electronic PCBs, electrical wiring and a digital display. The battery is removable and is a lithium polymer chemistry. The charging adapter and cable consist of electronic power supply components and electrical cabling. Dispose of this device in accordance with local regulations.

Contact your local Genea Biomedx service representative for more information.

	<p>NOTE:</p> <p>This Instrument is Subject to Laws Regarding the Disposal of Electronic Medical Equipment as Outlined in the WEEE Directive (2006/96/EC).</p>
---	--

4.4 Warnings & Faults: Troubleshooting

Problem	Cause	Solution
	Abnormal Lock Mechanism – Tank Unlocked	Power the device off and on using the Power On/Off Button. If this does not resolve the issue, attempt to reset using the emergency key, as detailed in Section "2.2.1". If the issue persists, please contact your local Genea Biomedx Service representative.
	Abnormal Lock Mechanism – Tank Locked	Power the device off and on. If this does not resolve the issue, contact your local Genea Biomedx Service representative. If immediate emergency access to the samples is required, please use the emergency key as detailed in Section "2.2.1".
Lock icon disappears	Immediately attempting to opening the lid after closing it can result in the latch not being properly positioned.	Attempt to reset using the emergency key, as detailed in Section "2.2.1". If this does not solve the issue, power the device on and off using the Power On/Off button. If the issue persists, please contact your local Genea Biomedx Service representative.
Router Connection Failed	Incorrect SSID or password parameter settings in IP configuration.	Confirm that the wireless network is functional, re-enter the correct SSID or password, and restart WI-FI.
Server Connection Failed	Failure in establishing a connection with the server for the first time.	Ensure that the server is functioning properly and that the server IP or server port parameters are correct. Then, restart both the server and WIFI to re-establish the connection.
Server Disconnected	Previously stable connection to the server lost.	Ensure that the server and network are functioning properly.
Device shuts down automatically after switching to battery, and at the same time, the battery LED light goes out automatically.	The battery is not powered on/activated.	Remove the battery and press and hold its side button. See Section "2.2.4" for further instructions.
The device does not wake up using the wake-up button but responds to screen taps.	The device has not entered sleep mode.	Power off the device and attempt a reset using the emergency key, as detailed in Section "2.2.1". If the issue persists, please contact your local Genea Biomedx service representative.

Problem	Cause	Solution
Abnormal screen colour	Abnormal screen LCD	Power off and then restart the device. If the issue persists, Contact the local Genea Biomedx service representative.
Touch functions not working	Abnormal touch screen or touch sensitive button behaviour.	Remove gloves and try touch elements or touch display with finger. If this resolves the issue, the glove type may not be compatible with the display. Otherwise, power off and then restart the device. If the issue persists, contact the local Genea
High/low position sensor fault	Sensor faulty or recalibration needed.	Contact the local Genea Biomedx service representative.
Upper probe temperature lower than lower probe	Recalibration of temperature sensor is required.	Contact the local Genea Biomedx service representative.
Forgotten Password or User has been Deleted	Administrator privileges required.	Contact the local administrator for a password reset or create new user.
Forgotten Administrator Password	Unable to access administrator only features.	In case of a forgotten password, users should contact the local Genea Biomedx service representative.
Restart during operation	Excessive memory usage during device operation triggers restart mechanism.	Waiting for device restart.



Operation Time	Event	Operator	Witness
05/31/2023 15:19:31	Lock		
05/31/2023 15:18:31	Unlock	001	
05/31/2023 15:16:20	Lock		
05/31/2023 15:15:19	Unlock	001	002



Local IP: _____

Server IP: _____

Server Port: _____

SSID: _____

Password: _____

Back Confirm

